

HNPS Advances in Nuclear Physics

Vol 26 (2018)

HNPS2018



Energy, Resolution and Efficiency Calibration of a LaBr₃(Ce) Scintillator

Eleni Ntalla, Alexandros Clouvas, Anastasia Savvidou

doi: [10.12681/hnps.1820](https://doi.org/10.12681/hnps.1820)

To cite this article:

Ntalla, E., Clouvas, A., & Savvidou, A. (2019). Energy, Resolution and Efficiency Calibration of a LaBr₃(Ce) Scintillator. *HNPS Advances in Nuclear Physics*, 26, 197–200. <https://doi.org/10.12681/hnps.1820>

Energy, Resolution and Efficiency Calibration of a LaBr₃(Ce) Scintillator

Eleni Ntalla^{1,2,*}, Alexandros Clouvas² and Anastasia Savidou¹

¹*Institute of Nuclear & Radiological Sciences & Technology, Energy & Safety, National Center for Scientific Research "Demokritos", Athens, Greece*

²*Department of Electrical and Computer Engineering, Aristotle University of Thessaloniki, Thessaloniki, Greece*

Abstract The last decade LaBr₃(Ce) scintillation detectors have become commercially available and have better scintillation properties (energy resolution, temperature performance, decay time, light yield and material density) when compared with NaI(Tl) scintillators. The aim of this work is the full calibration (energy, resolution and efficiency) of a 1.5x1.5 in LaBr₃(Ce) Canberra scintillator. Energy and resolution calibration were performed experimentally with the use of point sources with a source-detector distance at 22 cm. MCNPX simulations were performed in order to evaluate the efficiency calibration for three different source-detector geometries and then they were validated by the experimental efficiencies estimation.

Keywords gamma spectrometry, LaBr₃(Ce), calibration, MCNPX

INTRODUCTION

LaBr₃(Ce) scintillation detectors are very promising due to their high light yield (>65000 photons/MeV) that results in a better energy resolution compared to NaI(Tl) detector (<3% FWHM at ¹³⁷Cs), their decay time of 35 ns and their material density (5.29 g/cm³) [1, 2]. Due to their better scintillation properties, when compared with NaI(Tl) scintillators, they can substitute them in many applications. The main disadvantages of a LaBr₃(Ce) detector are the internal backgrounds of ¹³⁸La decaying to stable ¹³⁸Ba by electron capture and the ¹³⁸Ce decay by beta emission, which affect the background spectrum up to 1500 keV [3].

In this study, the full calibration (energy, resolution and efficiency) of a 1.5x1.5 in LaBr₃(Ce) Canberra scintillation detector is performed. For this purpose, two multiple gamma ray emitting sources (a large volume source and a large area source) as well as three point sources (²⁴¹Am, ⁶⁰Co and ¹⁵²Eu) were used.

Energy and resolution calibration were performed experimentally with the use of the point sources with a source–detector distance at 22 cm, by fitting several functions in both calibrations. MCNPX simulations were performed in order to evaluate the efficiency calibration for three different source-detector geometries and then validated by the experimental efficiencies estimation.

* Corresponding author, email: dalla@ipta.demokritos.gr

MATERIALS AND METHODS

Experimental Setup

The gamma spectrometry system is consisted of the following main parts:

- Detector unit: a Canberra scintillation detector LaBr₃(Ce) (Model LABR-1.5x1.5) with a 1.5x1.5 in crystal in a hermetically sealed aluminum housing, including a photomultiplier tube, an internal magnetic/light shield and a 14-pin connector (Fig.1)
- Electronics and acquisition unit: a digital signal processing unit (Osprey Digital Tube Base MCA) and a high voltage supply system (670 V).
- Lead shielding structure with thickness 5 cm

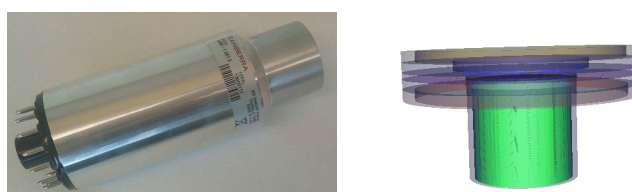


Fig. 1 The LaBr₃(Ce) detector (left) and MCNPX simulation of the gamma area source (right)

SPECTRW software [4] was used for spectrum analysis and MCNPX Monte Carlo code for efficiency evaluation by simulations (Fig.1).

The experimental data were obtained from two multiple gamma ray emitting sources (a large volume source and a large area source) and three point sources (²⁴¹Am, ⁶⁰Co and ¹⁵²Eu) (Table 1).

Isotope	T _{1/2} (d)	Reference Activity (Bq)			Source Uncertainty (%)		
		VS	AS	PS	VS	AS	PS
²¹⁰ Pb	8139.5	12300	12400	-	11.4	11.4	-
²⁴¹ Am	157753	1230	1180	351000	3.6	3.6	3
¹³⁷ Cs	11001.1	2600	1870	-	2.9	2.9	-
⁶⁰ Co	1923.55	3250	2190	384700	2.9	2.9	3

Table 1 Characteristics of radioactive sources used for the LaBr₃(Ce) detector calibration. The reference date for Volume Source (VS) and Area Source (AS) is 01/03/2007. The reference date for ²⁴¹Am and ⁶⁰Co point sources (PS) is 01/10/1995 and the reference date for ¹⁵²Eu point source (PS) is 01/03/2004

Each of the multiple ray emitting sources was adapted on an acetal holder that was attached on the detector surface (Fig.2).



Fig. 2 The acetal holder: the source side (left) and the detector side (right)

Internal Background of LaBr₃(Ce)

The internal background of LaBr₃(Ce) (Fig.3) was taken into account in all measurements and subtracted in all spectra.

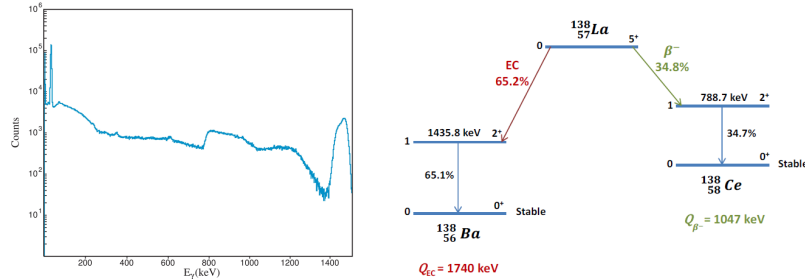


Fig. 3 Background spectra of LaBr₃(Ce): Internal activity of ¹³⁸La (T_{1/2} = 1011 y) and ²²⁷Ac (T_{1/2} = 21.77 y) in the energy range 0 – 1500 keV (acquisition time 54000 sec) and ¹³⁸La decay diagram

Energy and Resolution Calibration

The three point sources (²⁴¹Am, ⁶⁰Co and ¹⁵²Eu) were used in order to establish the relationship between the channel number and the photon energy (keV) (energy calibration) and the dependence of the Full Width Half Maximum (FWHM) (%) on the photon energy (keV) (resolution calibration) (Fig.4).

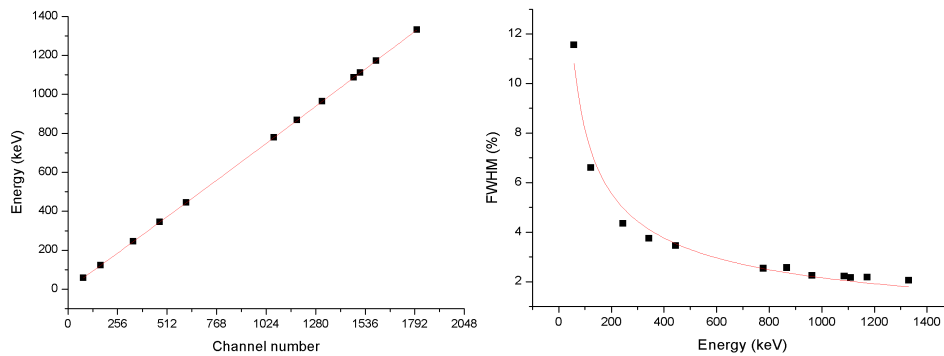


Fig. 4 Energy calibration (left) and resolution calibration (right) of the LaBr₃(Ce) scintillator

A 2nd order polynomial proved to be the best option for the energy calibration:

$$y = 1.047 \cdot 10^{-5} x^2 + 0.7194 x + 0.64, \text{ with adjusted } R^2 = 1$$

and a power curve for the resolution calibration: $y = 87.28 x^{-1/2} - 0.6$, with adjusted $R^2 = 0.98$.

Efficiency Calibration

For efficiency calibrations, the Absolute Full Energy Peak Efficiency (AFEPE) was evaluated for three different source-detector geometries. AFEPE relates the peak area to the number of gamma rays emitted by the source and depends upon the geometrical arrangement of source and detector [5].

The following source-detector geometries were studied:

- 1) Points sources (PS) at 22 cm from detector surface
- 2) Multiple gamma volume source (VS) adapted on the acetal holder

3) Multiple gamma area source (AS) adapted on the acetal holder

MCNPX simulations were performed for the above geometries and validated by the experimental efficiency calibrations (Fig.5-6). The black dots represent the MCNPX data and red dots the experimental data.

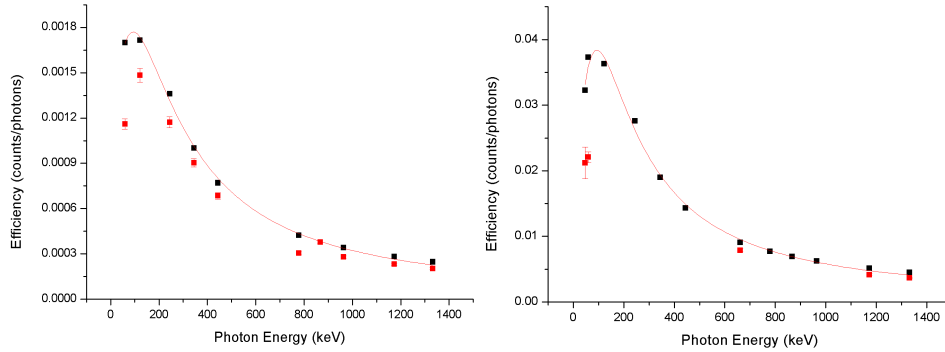


Fig. 5 Efficiency calibration curves for the geometries (PS) (left) and (VS) (right) with the corresponding selected fitting functions for the MCNPX data: $y = (2.874 x^{0.394}) / (7444 + x^{1.703})$, $R^2 = 0.998$ and $y = (38.413 x^{0.587}) / (9800 + x^{1.857})$, $R^2 = 0.995$

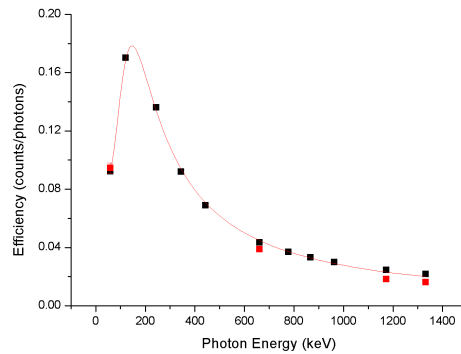


Fig. 6 Efficiency calibration curve for the geometry (AS) with the selected fitting function for the MCNPX data $y = (81.122 x^{2.780}) / (18 * 10^7 + x^{3.953}) + 3.318/x$, with $R^2 = 0.999$

CONCLUSIONS

In this study, a complete calibration of a Canberra 1.5x1.5 in LaBr₃(Ce) scintillator is presented. The bias observed between MCNPX simulations and experimental data can be attributed to the lack of the specific characteristics of the detector; only the generic characteristics were given from the manufacturer. Future work will be focused on the efficiency calibration optimization.

References

- [1] G. F. Knoll, John Wiley and Sons (1999)
- [2] F. Quarati et al., Nucl. Instr. Meth. Phys. Res. A 574, 1 (2007)
- [3] R. Nicolini et al., Nucl. Instr. Meth. Phys. Res. A 582, 2 (2007)
- [4] C. Kalfas et al., Nucl. Instrum. Methods Phys. Res. A 830 (2016)
- [5] G. Gilmore, John Wiley and Sons (2008)