


## HNPS Advances in Nuclear Physics

Vol 21 (2013)

HNPS2013

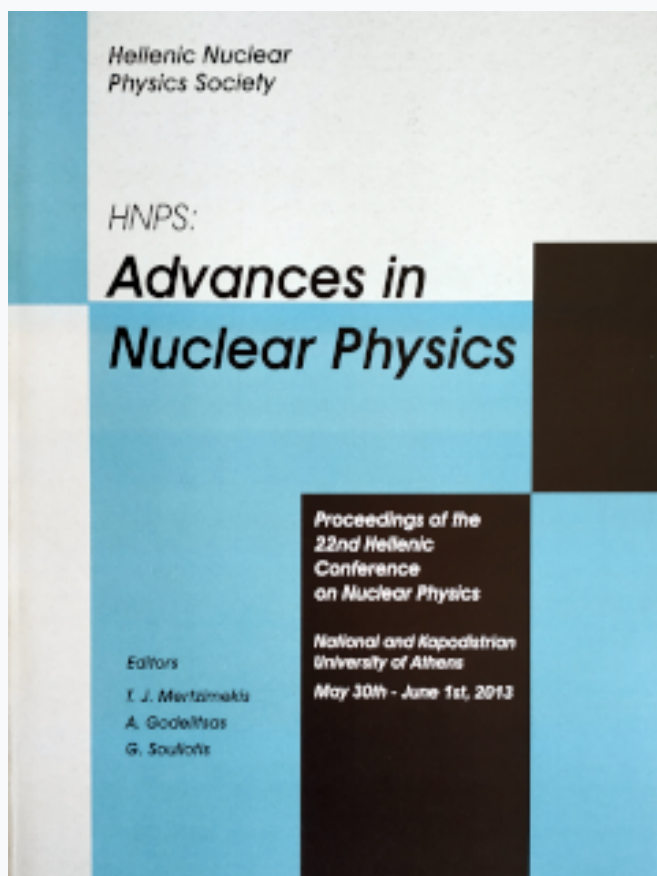

### Progress in radionuclide characterisation in marine sediments using an underwater gamma-ray spectrometer in $2\pi$ geometry

*E. G. Androulakaki, C. Tsabaris, M. Kokkoris, G. Eleftheriou, D. L. Patiris, F. Pappa, R. Vlastou*

doi: [10.12681/hnps.2000](https://doi.org/10.12681/hnps.2000)

#### To cite this article:

Androulakaki, E. G., Tsabaris, C., Kokkoris, M., Eleftheriou, G., Patiris, D. L., Pappa, F., & Vlastou, R. (2019). Progress in radionuclide characterisation in marine sediments using an underwater gamma-ray spectrometer in  $2\pi$  geometry. *HNPS Advances in Nuclear Physics*, 21, 29–32. <https://doi.org/10.12681/hnps.2000>

# Progress in radionuclide characterisation in marine sediments using an underwater gamma-ray spectrometer in $2\pi$ geometry

E.G. Androulakaki<sup>a,b</sup>, C. Tsabaris<sup>a</sup>, M. Kokkoris<sup>b</sup>, G. Eleftheriou<sup>a,b</sup>, D.L. Patiris<sup>a</sup>, F. Pappa<sup>a,b</sup>, R. Vlastou<sup>b</sup>

<sup>a</sup>*Institute of Oceanography, Hellenic Centre for Marine Research, 19013, Anavyssos, Greece*

<sup>b</sup>*Department of Physics, National Technical University of Athens, 15780, Zografou, Greece*

---

## Abstract

The *in-situ* gamma-ray spectrometry is a well suited method for seabed mapping applications, since it provides rapid results in a cost effective manner. Moreover, the *in-situ* method is preferable to the commonly applied laboratory measurements, due to its beneficial characteristics. Therefore, the development of *in-situ* systems for seabed measurements continuously grows. However, an efficiency calibration of the detection system is necessary for obtaining quantitative results in the full spectral range. In the present work, an approach for calculating the full-energy peak efficiency of an underwater *in-situ* spectrometer for measurements on the seabed is presented. The experimental work was performed at the coastal site of Vasilikos (Cyprus). The experimental full-energy peak efficiency of the *in-situ* was determined in the energy range 1400–2600 keV, by combining the *in-situ* and laboratory reference measurements. The experimental efficiency results were theoretically reproduced by means of Monte Carlo (MC) simulations, using the MCNP5 code.

*Keywords:* Targets Characterization, Ion Beams

---

## 1. Introduction

Radionuclide concentration measurements on marine sediments are traditionally performed using sampling techniques and spectrometric analysis in the laboratory. The widely applied method is the laboratory based gamma-ray spectrometry, since the majority of the natural and anthropogenic radionuclides can be detected from their gamma-ray lines. The laboratory method is not cost effective, since it requires manpower and instrumentation for sampling as well as laboratory facilities for the time-consuming procedures involved in the samples preparation. In addition, the laboratory method is applicable only at regions where the conventional grabbing techniques can successfully be employed (for instance non-rocky sea beds).

An alternative to the aforementioned difficulties, is the application of the *in-situ* gamma-ray spectrometry method. The benefits of the implementation of *in-situ* techniques for direct measurements on the seabed are well known, and a lot of effort has been devoted to the development of such detection systems [Jones, 2001]. During the last decades, several *in-situ* systems consisting of different types of detectors have been employed [Van Put 2004; Povinec et al., 1996; de Meijer et al., 2002] for aquatic and marine environment applications. Calibrations are carried out using appropriate laboratory facilities (e.g. special tank), reference calibration sources [Tsabaris et al. 2005] and Monte Carlo simulations [Maučec M., 2004; Vlastou et al., 2006; Bagatelas et al., 2010]. A review of the progress in developing techniques for *in-situ* measurements is summarized in the work of Jones [Jones 2001] and a recent updated status is also available [Thornton et al., 2013].

In this work an efficiency calibration of the *in-situ* system KATE [Tsabaris et al., 2008] was performed for measurements on the seabed in  $2\pi$  geometry. The system was deployed to acquire spectra in close contact with a specific seabed (the  $2\pi$  geometry) as well as in the seawater (the standard  $4\pi$  geometry). Additionally, a sediment sample was collected from a site adjacent to the deployment and analyzed in the laboratory. The activity concentrations (Bq/kg dry weight) on the sample were measured at the laboratory by means of high resolution gamma-ray spectrometry. The experimental full-energy peak efficiency of the *in-situ* system was

calculated in energies covering the interval 1460–2600 keV, by combining the *in-situ* measurements with the laboratory activity reference measurements. The efficiency results for the specific seabed were subsequently reproduced by implementing the MC MCNP5 code.

## 2. Experimental Setup and Field Work

The experimental work was performed at the coastal site of Vasilikos (Cyprus). The *in-situ* detection system utilized in the present application for the gamma-ray measurements on the seabed was developed at the Hellenic Centre for Marine Research [Tsabaris C., et al., 2004, 2005, Tsabaris C., et al., 2008]. The efficiency calibration for measurements on the seabed was held directly on the field by deploying the system in the sea to acquire spectra. For the sediment measurement the detector was situated in close contact with the seafloor ( $2\pi$  geometry measurement) to assure that high counting rates from the radionuclides present in the sediment are recorded. The system was subsequently deployed for an additional measurement in the seawater ( $4\pi$  geometry measurement). For this background measurement the detector was positioned well above the seabed, thus recording events present only in the seawater in  $4\pi$  geometry. This measurement was performed in order to estimate the contribution of radionuclides present in the seawater during the seabed measurement and properly subtract it. The contribution from each radionuclide is calculated by peak integration in the spectrum acquired in the  $4\pi$  geometry measurement (seawater measurement). The calculated total count rate in each photopeak is multiplied by a factor of 1/2, and this quantity is subsequently subtracted from the count rate determined in the corresponding peaks of the sediment spectrum ( $2\pi$  geometry measurement).

Moreover, a sediment sample was collected from a site adjacent to the deployment. The grabbing technique was utilized for the sediment sample collection from the seafloor, thus a collection from a maximum depth of 15 cm was achieved. The collected sample was dried out and homogenized prior to the preparation of the final sample in the standard geometry for environmental measurements. The reference gamma-ray spectroscopy measurement was held at the facilities of the National Technical University of Athens (NTUA). Additionally, theoretical estimations were performed using the MCNP5 code to reproduce the experimental efficiency values.

In this work, the previously [Androulakaki et al., 2012] described methodology for the efficiency calculation at the energy 1460 keV ( $^{40}\text{K}$  gamma-ray line), is expanded to the energies 1460–2600 keV. In this way, activity concentration calculations using the *in-situ* method are expanded, making possible the quantification of the radionuclides  $^{208}\text{Tl}$  (2614 keV) and  $^{214}\text{Bi}$  (1765 keV) present on the seabed.

## 3. Analysis and Results

The volumetric efficiency of the *in-situ* system for measurements on the seabed,  $\epsilon_V$  (in units of lt), was deduced combining the *in-situ* acquired peak analysis data with the reference concentration activities (as deduced from the laboratory measurement in units of Bq/lt). Special attention was paid to employ proper analysis techniques in cases where in the analyzed peaks contributed more than one photopeaks attributed to radionuclides with neighboring gamma-ray lines (e.g. a total emission probability that equals the sum of the intensities of each gamma-ray line of the radionuclide  $^{214}\text{Bi}$  contributing to the peak at 1765 keV was considered). The efficiency results (simulated and experimental) are depicted in Fig. 1 as a function of the gamma-ray energies.

The experimental uncertainty was found 10% for the calculated efficiency at the energy of 2614 keV ( $^{208}\text{Tl}$ ) and 1461 keV ( $^{40}\text{K}$ ) and 20% at 1765 keV ( $^{214}\text{Bi}$ ). The observed uncertainties are attributed to the low activity concentrations of the studied area. The simulation results are in satisfactory agreement (less than 7% relative deviation) with the experimental ones within statistical uncertainties. The accuracy of the obtained results, render the simulations as a powerful tool to be utilized, especially for seabed applications where the variations in the seafloor properties influence the detectors efficiency. A theoretical study of the detection efficiency sensitivity to geophysical sediment parameters is thus considered, as the following step to the present work. Moreover, it is crucial to expand the efficiency calibration in the lower energy region between 300–1460 keV. In order to achieve this goal it is necessary to obtain more experimental data by

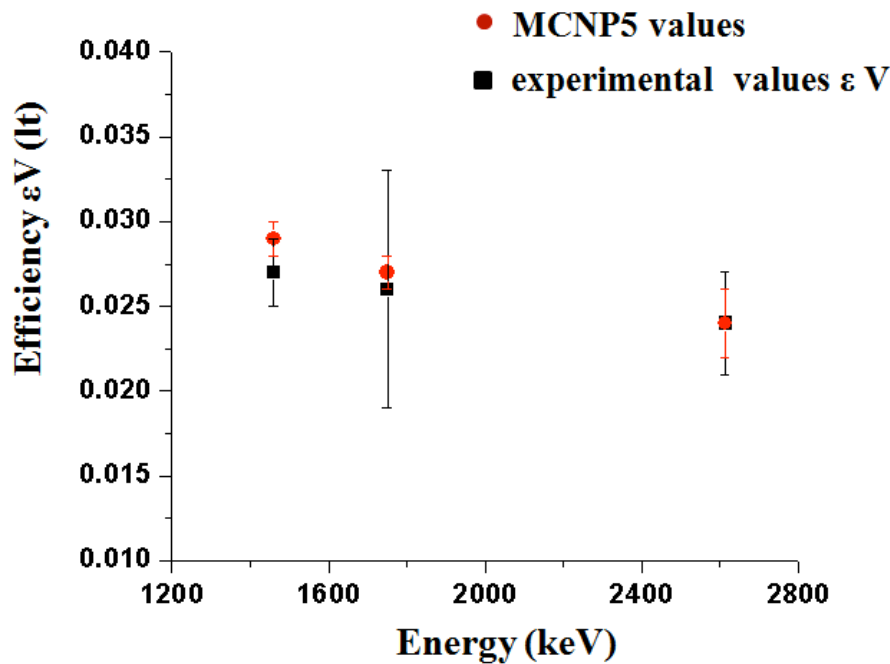


Figure 1: The experimental and simulated efficiency of the *in-situ* system for seabed applications

deploying the in-situ system in marine ecosystems containing Naturally Occurring Radioactive Materials (NORM). Future deployments are organized in such environments, in order to assure that high quality spectra are acquired.

### Acknowledgments

The authors would like to thank the International Atomic Energy Agency for the financial support of the campaign within the RER/7/003 project. Mr Christos Tsabaris would like to acknowledge Mr Jan Scholten from IAEA for supporting field work during the campaign as well as Mr Panicos Demetriades from the Department of Labour Inspection in Cyprus for the hospitality and his support during the experimental work in the field.

### References

- Androulakaki E.G., Tsabaris C., Kokkoris M., Eleftheriou G., Patiris D.L., Vlastou R., 2012. *In situ Gamma-Ray Measurements of Marine Sediment using Monte Carlo Simulation*, Proceedings of the 21st Hellenic Conference on Nuclear Physics, pg. 139-144.
- Bagatelas, C., Tsabaris, C., Kokkoris, M., Papadopoulos, C.T., Vlastou, R., 2010. *Determination of marine gamma activity and study of the minimum detectable activity (MDA) in 4pi geometry based on Monte Carlo simulation*, Environ. Monit. Asses. 165,159-168
- van Put, P., Debauche, A., De Lellis, C., Adam, V., 2004. *Performance level of an autonomous system of continuous monitoring of radioactivity in seawater*, J. Environ. Rad. 72, 177-186
- Thornton B., Ohnishi S., Ura T., Odano N., Fujita T., 2013. *Continuous measurement of Radionuclide distribution off Fukushima using a towed sea-bed gamma ray spectrometer*, Deep-Sea Research I 79, 10-19

- Tsabaris C. and Thanos I., 2004. An underwater sensing system for monitoring radioactivity in the marine environment, *Mediterranean Marine Science*, 5, 125-131
- Tsabaris C., 2008. Monitoring natural and artificial radioactivity enhancement In the Aegean Sea using floating measuring systems, *Radiat. Prot. Dosim.*, 66, 1599-1603.
- Tsabaris, C., Vlachos, D.S., Papadopoulos, C.T., Vlastou, R., Kalfas, C.A., 2005. Set up and application of an underwater  $\gamma$ -ray spectrometer for radioactivity measurements, *Mediterranean Marine Science*, 6, 35-40.
- Jones D.G., 2001. Development and application of marine gamma-ray measurements: a review, *J. Environ. Rad.* 53, 313333
- Povinec P.P., Osvath I., Baxter M.S., 1996. *Underwater Gamma-spectrometry with and NaI(Tl) Detectors*, *Appl. Radiat. Isot.*, 47, 1127
- De Meijer R.J., Limburg J., Venema L.B., 2002. Natural radioactivity in monitoring waste disposals, *Phys. Scr.* 97, 139147
- Maučec M., de Meijer R.J., Rigollet C., Hendriks P.H.G.M., Jones D.G., 2004. *Detection of radioactive particles offshore by  $\gamma$ -ray spectrometry Part I: Monte Carlo assessment of detection depth limits*, *Nuclear Instruments and Methods* 525, 593-609
- Vlastou R., Ntziou I.Th., Kokkoris M., Papadopoulos C.T. and Tsabaris C., 2006. *Monte Carlo simulation of  $\gamma$ -ray spectra from natural radionuclides recorded by a NaI detector in the marine environment*, *Appl. Radiat. Isot.*, 64, 116123